


Peen mark to clearly identify position of T1 & T2 in melt flow

Duplex Thermocouple Connector
 To be clearly identified with T1 & T2.

IMPORTANT NOTE:
 Please note position of T2 (above) and polarity of plug pins.

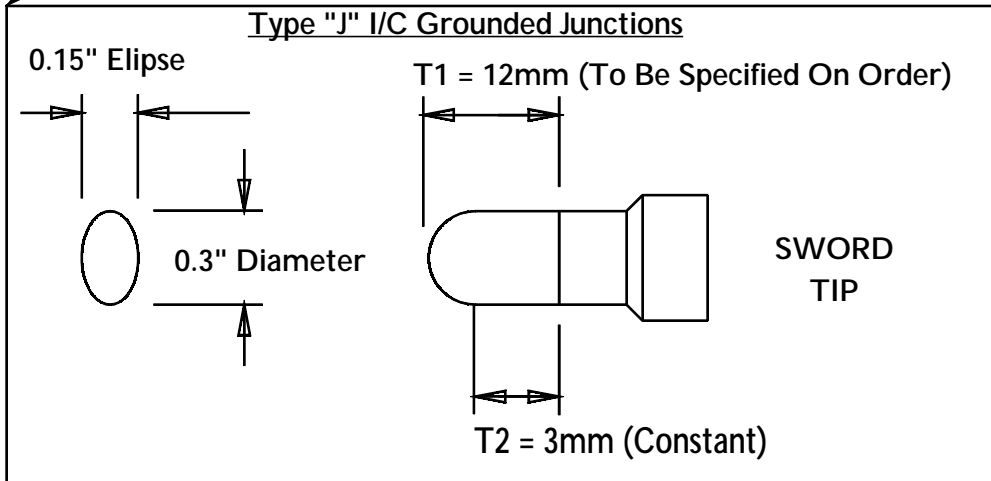

Production Test:
 Each unit to be pressure tested at 10,000psi.

DIMENSIONS	
A =	80.0mm
B =	12.7 (1/2")
C =	63.5 (2.5")
D =	72.2mm
E =	12.20 (0.48)
F =	10.49±0.03 (0.413±0.001)
G =	7.77±0.03 (0.306±0.001)
H =	5.54±0.12 (0.218±0.005)
J =	12.7 DIA' (0.50)

Terwin Instruments Limited

Tollemache Road,
 Spittlegate Level Industrial Estate,
 Grantham,
 Lincolnshire.
 NG31 7UH
 Tel. +44 (0) 1476 565797
 Fax. +44 (0) 1476 590139

DRAWN	G.W.
DATE	27.10.99
CHECKED	M.F.
APPROVED	B Cleland

DRG. NO.	MCD/TC/0292
TITLE	Cryovac Sealed Air (New Zealand) EXTRUSION THERMOCOUPLE

CAD REF.	Ti292
MATERIAL:	BOLT - 316 STAINLESS STEEL
TOLERANCES:	±0.1 U.O.S. +1 / -0 Degree

(B)	1 May 2001	Duplex plug mounted incorrectly	B Cleland
ISS	DATE	DESCRIPTION	APP'D